


How to Collect Blood Using the PAXgene™ Blood RNA Tube

For Molecular Diagnostic Testing

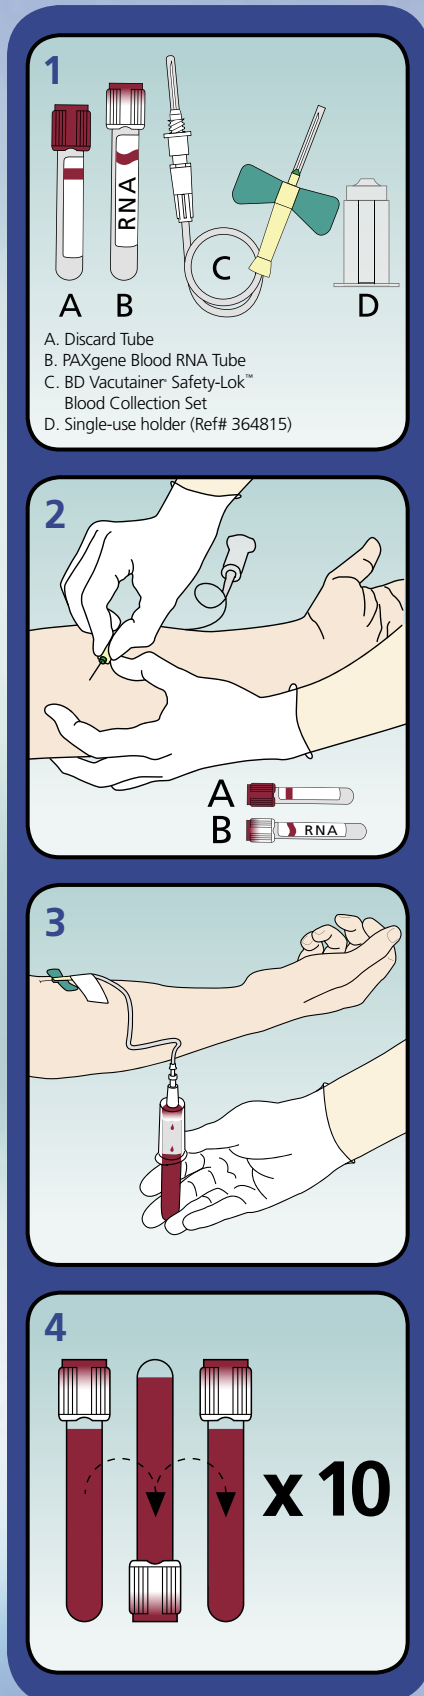

Required Items:

- 1a. Ensure that the PAXgene Blood RNA Tube (B) is at room temperature (18°C-25°C) prior to use and properly labeled with patient identification.
- 1b. If the PAXgene Blood RNA Tube is the only tube to be drawn, a small amount of blood should be drawn into a "Discard Tube" (A) prior to drawing blood into the PAXgene Blood RNA Tube. Otherwise, the PAXgene Blood RNA Tube should be the last tube drawn in the phlebotomy procedure.

Venipuncture:

2. Using a BD Vacutainer® Safety-Lok™ Blood Collection Set (C), collect blood into the PAXgene Blood RNA Tube using your institution's recommended standard procedure for venipuncture.

Blood Collection:

- 3a. Hold the PAXgene Blood RNA Tube vertically, below the blood donor's arm, during blood collection.
- 3b. Allow at least 10 seconds for a complete blood draw to take place. Ensure that the blood has stopped flowing into the tube before removing the tube from the holder. (See Figure 1)

After Blood Collection:

- 4a. Gently invert the PAXgene Blood RNA Tube 8 to 10 times.
- 4b. Store the PAXgene Blood RNA Tube upright at room temperature (18°C-25°C) or at 4°C.*

Before Blood Collection



Ref# 762165

After Blood Collection



BD Vacutainer® Safety-Lok™ Blood Collection Set

Ref# 367281 North America
Ref# 367286 Other Countries

BD Customer Service/Orders:
888.237.2762 (North America)
32.53.720.337 (Europe)

PreAnalytiX

A QIAGEN / BD Company

www.PreAnalytiX.com



*Refer to PAXgene® Blood RNA Tube handbook.
PAXgene and PreAnalytiX are registered trademarks of PreAnalytiX, Hombrechtikon, CH ©2005 PreAnalytiX GmbH
BD and all other trademarks are the property of Becton, Dickinson and Company. ©2005 BD
Printed in USA 05/05 VS5933-1